



Date 12.01.2016

TEST REPORT NO. *CBC-001/2016*

Page 1 of 15

Subject of testing: *Ramp*Classification according to
PN-EN ISO 9999:2011 : 18 30 15Type / Model: *SC 045*
SC 090
SC 120
*SC 150*SN.: *D10615048*
D10315045
D10415056
*D10515063*Manufacturer: *MOBILEX A/S*
Grønlandsvej 5
DK-8660 Skanderborg

Number of specimens: 4

Applicant: *A-Net s.c.*
93-469 Łódź,
*ul. Łaskowice 174*Kind of testing *Testing scope according to application of Client*
*Mechanical testing according to PN-EN 12182:2012;*Test started: *4.01.2016*Test finished: *12.01.2016*

Approved by:

DYREKTOR

mgr inż. Andrzej Tkaczyk

Special comments / enclosures:

Copyright © 2012 by Centre for Testing and Certification (applicable to report form)

Test results refer only to tested units.

Test results reported here are not applicable to the further modifications of the product affecting its structure, material or technology.

This test report shall be neither copied differently as in the whole nor be published without written consent of the Laboratory.




TESTING

NORMATIVE REFERENCES

PN-EN 12182:2012

Technical aids for disabled persons – General requirements and test methods

PHOTO OF PRODUCT

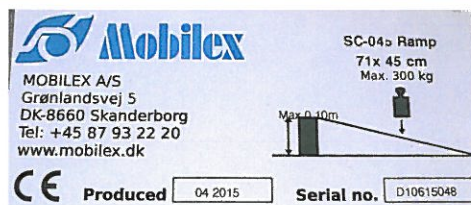

CHARAKTERISTICS OF PRODUCT

Name of product: SC-045 Ramp	SN: D10615048	Max. loading: 300 kg	Mass of product: 4,13 kg
---------------------------------	------------------	-------------------------	-----------------------------

Dimensions:

Composite : 457 x 365 x 85 mm

Spread out: 457 x 706 x 64 mm

Material:

aluminum, steel, plastic

TEST RESULTS according to PN-EN 12182 : 2012

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Test result	Opinion	Comments
4.1	4.8, 5.2, 5.4.2, 5.5, 6, 8.2.1, 9.4, 10, 22, 24 i EN 1441	Risk analysis		--	N/T	
4.2	V/I	Expected characteristics and technical documentation		Conf.	Pos.	
4.3	EN ISO 14155	Clinic assessment		--	N/T	
4.4	V/I	Technical support which can be dismantled		Conf.	Pos.	
4.5	V/I	Single use connections		Conf.	Pos.	
4.6	V/I	Boundary values of user weight		Conf.	Pos.	
4.7	V/I	Immobilising means		--	N/A	
4.8	V/I, C5	Suitability of the product for people with cognitive impairment		--	N/T	
		The presence of the description in the manufacturer's documentation		--	N/T	
		Materials				
5.1	EN 60601-1-9	Recycling		--	N/T	
5.2	V/I, B 5.2	Flammability		--	N/A	
5.2.2	V/I	Upholstered parts, mattresses, bed bases and bedding		--	N/A	
5.2.3	V/I, EN 1021	Upholstered parts		--	N/A	
5.2.4	V/I, EN 597	Mattresses and bed bases		--	N/A	
5.2.5	V/I, EN ISO 12952	Bedding		--	N/A	
5.2.6	V/I, EN 60695-11-10	Moulded parts		--	N/A	
5.3	EN ISO 10993-1 Annex. D	Biological conformity and toxicity		--	N/T	
5.4	V/I	Contaminants and residues		--	N/A	
5.5	V/I, B.5.5.1	Microbiological infections and contamination	Cleaning	Conf.	Pos.	
	V/I, B.5.5.1		Disinfection	--	N/A	
	V/I, EN ISO 22442-1 B.5.5.2		Animal tissue	--	N/A	
5.6	EN ISO 9227	Resistance to corrosion		--	N/T	
6		Emitted sound and vibration				
6.1	EN ISO 3746 B6	Noise and vibration		--	N/A	
6.2	EN ISO 3746	Sound levels and frequencies of audible warning devices		--	N/A	
Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Real value	Test result	Comments
6.3	EN ISO 3746	Feedback		--	N/A	
7	EN 60601-1-2 7.2, 7.3, 7.4	Electromagnetic compatibility		--	N/A	
8		Electrical safety		--	N/A	
9	V/I	Overflow, spillage, leakage, and ingress of liquids		--	N/A	
10	V/I. Measur.	Surface temperature		--	N/A	$t^{\circ} \leq 41^{\circ}C$ ■ requirement does not concern heat of direct solar radiation - PN-EN 12182, clause 10a ■ requirement concerns only persons with insensitiveness of skin (who do not feel heat) - PN-EN 12182, clause 10d
11	V/I	Sterility		--	N/A	

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters	Real value	Test result	Comments
12	V/I. Measur.	Safety of moving parts	Conf.	Pos.	Note in service manual
13	V/I. Measur.	Prevention of traps for parts of the human body	Conf.	Pos.	Note in service manual
14	V/I	Folding and adjusting mechanisms	Conf.	Pos.	Note in service manual
15	V/I. Measur.	Carrying handles	--	N/A	
16	V/I. Measur.	Assistive products which support or suspend users	Conf. *)	Pos.	loading 1,5x300kg=450kg, 70sek. 1000 cycles, 300kg
17	V/I. Measur.	Portable and mobile assistive products	--	N/A	
18	V/I, B 18	Surfaces, corners, edges and protruding parts	Conf.	Pos.	
19	B 19	Hand held assistive products	--	N/A	
20	B 20	Small Parts	Conf.	Pos.	
21	V/I. Measur. EN 60601-1	Stability	--	N/A	
22	B 22, V/I	Forces in soft tissues of the human body	--	N/A	
23	V/I. EN 614-1	Ergonomic principles	--	N/T	The requirements relate to the design process

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters	Real value	Test result	Comments
24	V/I	Requirements for information supplied by the manufacturer			
24.1		General	--	N/T	
24.2		Instructions for use	--	N/T	
24.2.1	V/I	Pre-sale Information			
		a) information on how to obtain the user information in a format appropriate for use by people with visual, reading or cognitive disabilities	--	N/T	
		b) all information shall as far as possible be available in Pictogram	--	N/T	
		c) a description of the intended use and the intended environment;	--	N/T	
		d) maintenance instructions, if applicable;	--	N/T	
		e) if an assistive product is intended to be cleaned, a description of the method and suitable cleaning materials, including precautions needed to avoid corrosion, if applicable;	--	N/T	
		f) if an assistive product is intended to be disinfected, a description of the method and suitable materials, including any precautions needed to avoid corrosion, if applicable;	--	N/T	
		g) the overall dimensions (width, length and height) of the assistive product, expressed in millimetres, and its mass, expressed in kilograms, when it is ready for use and, if applicable, when it is folded or dismantled	--	N/T	
24.2.1	V/I	h) the mass expressed in kilograms if the assistive product can be dismantled or has any removable parts that has a mass which is heavier than 10 kg;	--	N/T	
		i) if the assistive product is supposed to be used in combination with other products, the manufacturer shall state to which products, and how this can be done in a safe way;	--	N/T	
		j) warning about dangerous combinations of devices (e.g. cushions for the prevention of decubitus ulcers often only work on correct seat surface) and combinations of flame resistant and non-flame resistant material;	--	N/T	
		k) a list of accessories, detachable parts and materials that the manufacturer has determined as being intended for use with the assistive product	--	N/T	
		l) if a programmable controller is fitted, information on the method of programming, the competence required to carry out the programming and the effects on performance	--	N/T	
		m) operator control adjustments	--	N/T	
		n) whether and how the assistive product can be folded or dismantled to assist in storage or transport	--	N/T	
		o) instructions regarding transport of the assistive product (e.g. in a car or aeroplane)	--	N/T	
		p) measured sound power level	--	N/T	

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters	Real value	Test result	Comments
24.2.2	V/I	User information			
		User information shall be provided by the manufacturer with each assistive product. Information shall contain all pre-sale warnings and informations and the following as applicable for each assistive product:	--	N/T	
		a) the location and the type of identification number/word on the assistive product shall be given for the unique identification number of the assistive product	--	N/T	
		b) the intended user	--	N/T	
		c) any adjustment or settings required before the assistive product can be used and information on how adjustments or settings affect the assistive product	--	N/T	
		d) information on adjustment possibilities and the competence required to carry out these adjustments	--	N/T	
		e) instructions on operation of all controls	--	N/T	
		f) the battery type and nominal voltage	--	N/T	
		g) instructions for battery maintenance	--	N/T	
		h) instructions for operating the battery charger, including warnings regarding any potential safety hazards (e.g. a possibility of gas accumulating in the charging area);	--	N/T	
		i) instructions on dismantling and re-assembly of the assistive product or any removable parts;	--	N/T	
		j) the positions of points where the component parts can be gripped for safe moving and handling and/or a method for handling during dismantling, assembly or carrying;	--	N/T	
		k) a warning if surface temperatures can increase / decrease when exposed to external sources of heat or cold (e.g. sunlight, outdoor environment);	--	N/T	
		l) a warning if the assistive product might disturb the operation of devices in its environment that emit electromagnetic fields (e.g. alarm systems of shops, automatic doors, etc.);	--	N/T	
		m) a warning if the performance of the assistive product can be influenced by electromagnetic fields {e.g. those emitted by portable telephones, electricity generators or high power sources};	--	N/T	
		n) if the intended purpose of an assistive product cannot be met without a hazard {e.g. holes, V-shaped opening}, a warning and instructions on how to operate the assistive product safely;	--	N/T	
		o) if the intended purpose of an assistive product cannot be met without a hazard due to moving parts such as squeezing, a warning and instructions on how to operate the assistive product safely;	--	N/T	
		p) the level of resistance to ignition of materials and assemblies;	--	N/T	
24.2.2	V/I	q) information on the recycling of used batteries and other parts of the assistive product;	--	N/T	
		r) expected lifetime of the assistive product.	--	N/T	
		- It is recommended to include instructions on how to solve simple problems for the ease of use.	--	N/T	
24.2.3	V/I	Service information			
		The service information shall contain all the pre-sale information, user information and instructions necessary for the maintenance, adjustment and repair of the assistive product and for the replacement of parts.	--	N/T	
		The service information shall contain all the pre-sale information and the user information.	--	N/T	
		The service information shall be sufficiently detailed concerning preventive inspection, maintenance and calibration, including the frequency of such maintenance.	--	N/T	
		The service information shall provide information for the safe performance of such routine maintenance necessary to ensure the continued safe use of the assistive product.	--	N/T	
		Additionally, the service information shall identify the parts on which preventive inspection and maintenance shall be performed by service personnel, including the periods to be applied and details about the actual performance of such maintenance.	--	N/T	

Require ments accordi ng to clause	Test method accordi ng to clause	Checked characteristics/assemblies/parameters	Real valu e	Test result	Com ments
24.3	V/I	Labelling	--	N/T	
		- year of production for the product	--	N/T	
		- Detachable parts of an assistive product with a mass of more than 10 kilograms shall be marked with the actual mass on the part.	--	N/T	
		- Symbol for use in the labelling of medical devices shall be in accordance with EN 980	--	N/T	
25	V/I	Packaging	--	N/T	Note 1

Pos. – positive; Neg – negative; N/T – not tested; N/A – not applicable; N/R – not required, N/O – not occurred, V/I.- visual inspection, Conf.- conformed.

NOTE 1: Assessment of package, clause 25 concerns risk of threats caused by improper protection against damage, fall or impurity during storage and transport to place of use

NOTE 2: Conformity assessment of product according to standard requirements refer to the scope of mechanical tests ordered by client

NOTE 3: During visual inspection before testing any visible defects that can have an effect on test results were not stated.

NOTE 4: Sample/object for testing was delivered to the Laboratory by the Orderer.

CONCLUSIONS:

Testing object **conforming** with requirements of PN-EN 12182:2012


TESTING

NORMATIVE REFERENCES

PN-EN 12182:2012

Technical aids for disabled persons – General requirements and test methods

PHOTO OF PRODUCT

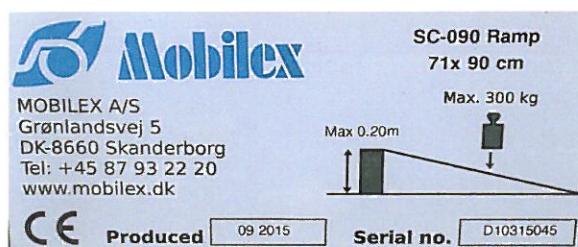

CHARAKTERISTICS OF PRODUCT

Name of product: SC-090 Ramp	SN: D10315045	Max. loading: 300 kg	Mass of product: 8,23 kg
--	-------------------------	--------------------------------	------------------------------------

Dimensions:

Composite :	916 mm x 366 mm x 86 mm
Spread out:	916 mm x 705 mm x 60 mm

Material:

aluminum, steel, plastic

TEST RESULTS according to PN-EN 12182 : 2012

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Test result	Opinion	Comments
4.1	4.8, 5.2, 5.4.2, 5.5, 6, 8.2.1, 9.4, 10, 22, 24 i EN 1441	Risk analysis		--	N/T	
4.2	V/I	Expected characteristics and technical documentation		Conf.	Pos.	
4.3	EN ISO 14155	Clinic assessment		--	N/T	
4.4	V/I	Technical support which can be dismantled		Conf.	Pos.	
4.5	V/I	Single use connections		Conf.	Pos.	
4.6	V/I	Boundary values of user weight		Conf.	Pos.	
4.7	V/I	Immobilising means		--	N/A	
4.8	V/I, C5	Suitability of the product for people with cognitive impairment		--	N/T	
		The presence of the description in the manufacturer's documentation		--	N/T	
		Materials				
5.1	EN 60601-1-9	Recycling		--	N/T	
5.2	V/I, B 5.2	Flammability		--	N/A	
5.2.2	V/I	Upholstered parts, mattresses, bed bases and bedding		--	N/A	
5.2.3	V/I, EN 1021	Upholstered parts		--	N/A	
5.2.4	V/I, EN 597	Mattresses and bed bases		--	N/A	
5.2.5	V/I, EN ISO 12952	Bedding		--	N/A	
5.2.6	V/I, EN 60695-11-10	Moulded parts		--	N/A	
5.3	EN ISO 10993-1 Annex. D	Biological conformity and toxicity		--	N/T	
5.4	V/I	Contaminants and residues		--	N/A	
5.5	V/I, B.5.5.1	Microbiological infections and contamination	Cleaning	Conf.	Pos.	
	V/I, B.5.5.1		Disinfection	--	N/A	
	V/I, EN ISO 22442-1 B.5.5.2		Animal tissue	--	N/A	
5.6	EN ISO 9227	Resistance to corrosion		--	N/T	
6		Emitted sound and vibration				
6.1	EN ISO 3746 B6	Noise and vibration		--	N/A	
6.2	EN ISO 3746	Sound levels and frequencies of audible warning devices		--	N/A	
Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Real value	Test result	Comments
6.3	EN ISO 3746	Feedback		--	N/A	
7	EN 60601-1-2 7.2, 7.3, 7.4	Electromagnetic compatibility		--	N/A	
8		Electrical safety		--	N/A	
9	V/I	Overflow, spillage, leakage, and ingress of liquids		--	N/A	
10	V/I. Measur.	Surface temperature		--	N/A	$t \leq 41^{\circ}\text{C}$ ■ requirement does not concern heat of direct solar radiation - PN-EN 12182, clause 10a ■ requirement concerns only persons with insensitiveness of skin (who do not feel heat) - PN-EN 12182, clause 10d
11	V/I	Sterility		--	N/A	

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters	Real value	Test result	Comments
12	V/I. Measur.	Safety of moving parts	Conf.	Pos.	Note in service manual
13	V/I. Measur.	Prevention of traps for parts of the human body	Conf.	Pos.	Note in service manual
14	V/I	Folding and adjusting mechanisms	Conf.	Pos.	Note in service manual
15	V/I. Measur.	Carrying handles	Conf.	Pos.	loading 160N
16	V/I. Measur.	Assistive products which support or suspend users	Conf. *)	Pos.	loading 1,5x300kg=450kg, 70sek. 1000 cycles, 300kg
17	V/I. Measur.	Portable and mobile assistive products	--	N/A	
18	V/I, B 18	Surfaces, corners, edges and protruding parts	Conf.	Pos.	
19	B 19	Hand held assistive products	--	N/A	
20	B 20	Small Parts	Conf.	Pos.	
21	V/I. Measur. EN 60601-1	Stability	--	N/A	
22	B 22, V/I	Forces in soft tissues of the human body	--	N/A	
23	V/I. EN 614-1	Ergonomic principles	--	N/T	The requirements relate to the design process

*) Deformation – 8 mm, Elastic deformation – 8 mm, sustained deformation – 0 mm

Pos. – positive; Neg – negative; N/T – not tested; N/A – not applicable; N/R – not required, N/O – not occurred, V/I.- visual inspection, Conf.- conformed.

NOTE 1: Assessment of package, clause 25 concerns risk of threats caused by improper protection against damage, fall or impurity during storage and transport to place of use

NOTE 2: Conformity assessment of product according to standard requirements refer to the scope of mechanical tests ordered by client

NOTE 3: During visual inspection before testing any visible defects that can have an effect on test results were not stated.

NOTE 4: Sample/object for testing was delivered to the Laboratory by the Orderer.

CONCLUSIONS:

Testing object **conforming** with requirements of PN-EN 12182:2012

TESTING

NORMATIVE REFERENCES

PN-EN 12182:2012

Technical aids for disabled persons – General requirements and test methods

PHOTO OF PRODUCT



MOBILEX A/S
Grønlandsvej 5
DK-8660 Skanderborg
Tel: +45 87 93 22 20
www.mobilex.dk



Produced

09 2015


Serial no.

D10415056

SC-120 Ramp
71x 120 cm

Max. 300 kg

Max 0.25m



CHARAKTERISTICS OF PRODUCT

Name of product: SC-120 Ramp	SN: D10415056	Max. loading: 300 kg	Mass of product: 11,13 kg
Dimensions:			
Composite :	1224 mm x 365 mm x 86 mm		
Spread out:	1224 mm x 708 mm x 60 mm		
Material:	aluminum, steel, plastic		

TEST RESULTS according to PN-EN 12182 : 2012

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Test result	Opinion	Comments
4.1	4.8, 5.2, 5.4.2, 5.5, 6, 8.2.1, 9.4, 10, 22, 24 i EN 1441	Risk analysis		--	N/T	
4.2	V/I	Expected characteristics and technical documentation		Conf.	Pos.	
4.3	EN ISO 14155	Clinic assessment		--	N/T	
4.4	V/I	Technical support which can be dismantled		Conf.	Pos.	
4.5	V/I	Single use connections		Conf.	Pos.	
4.6	V/I	Boundary values of user weight		Conf.	Pos.	
4.7	V/I	Immobilising means		--	N/A	
4.8	V/I, C5	Suitability of the product for people with cognitive impairment		--	N/T	
		The presence of the description in the manufacturer's documentation		--	N/T	
		Materials				
5.1	EN 60601-1-9	Recycling		--	N/T	
5.2	V/I, B 5.2	Flammability		--	N/A	
5.2.2	V/I	Upholstered parts, mattresses, bed bases and bedding		--	N/A	
5.2.3	V/I, EN 1021	Upholstered parts		--	N/A	
5.2.4	V/I, EN 597	Mattresses and bed bases		--	N/A	
5.2.5	V/I, EN ISO 12952	Bedding		--	N/A	
5.2.6	V/I, EN 60695-11-10	Moulded parts		--	N/A	
5.3	EN ISO 10993-1 Annex. D	Biological conformity and toxicity		--	N/T	
5.4	V/I	Contaminants and residues		--	N/A	
5.5	V/I, B.5.5.1	Microbiological infections and contamination	Cleaning	Conf.	Pos.	
	V/I, B.5.5.1		Disinfection	--	N/A	
	V/I, EN ISO 22442-1 B.5.5.2		Animal tissue	--	N/A	
5.6	EN ISO 9227	Resistance to corrosion		--	N/T	
6		Emitted sound and vibration				
6.1	EN ISO 3746 B6	Noise and vibration		--	N/A	
6.2	EN ISO 3746	Sound levels and frequencies of audible warning devices		--	N/A	
Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Real value	Test result	Comments
6.3	EN ISO 3746	Feedback		--	N/A	
7	EN 60601-1-2 7.2, 7.3, 7.4	Electromagnetic compatibility		--	N/A	
8		Electrical safety		--	N/A	
9	V/I	Overflow, spillage, leakage, and ingress of liquids		--	N/A	
10	V/I. Measur.	Surface temperature		--	N/A	$t \leq 41^{\circ}\text{C}$ ■ requirement does not concern heat of direct solar radiation - PN-EN 12182, clause 10a ■ requirement concerns only persons with insensitiveness of skin (who do not feel heat) - PN-EN 12182, clause 10d
11	V/I	Sterility		--	N/A	

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters	Real value	Test result	Comments
12	V/I. Measur.	Safety of moving parts	Conf.	Pos.	Note in service manual
13	V/I. Measur.	Prevention of traps for parts of the human body	Conf.	Pos.	Note in service manual
14	V/I	Folding and adjusting mechanisms	Conf.	Pos.	Note in service manual
15	V/I. Measur.	Carrying handles	Conf.	Pos.	loading 220 N
16	V/I. Measur.	Assistive products which support or suspend users	Conf. *)	Pos.	loading 1,5x300kg=450 kg, 70sek. 1000 cycles, 300 kg
17	V/I. Measur.	Portable and mobile assistive products	--	N/A	
18	V/I, B 18	Surfaces, corners, edges and protruding parts	Conf.	Pos.	
19	B 19	Hand held assistive products	--	N/A	
20	B 20	Small Parts	Conf.	Pos.	
21	V/I. Measur. EN 60601-1	Stability	--	N/A	
22	B 22, V/I	Forces in soft tissues of the human body	--	N/A	
23	V/I. EN 614-1	Ergonomic principles	--	N/T	The requirements relate to the design process

*) Deformation – 12 mm, elastic deformation – 12 mm, sustained deformation – 0 mm

Pos. – positive; Neg – negative; N/T – not tested; N/A – not applicable; N/R – not required, N/O – not occurred, V/I.- visual inspection, Conf.- conformed.

NOTE 1: Assessment of package, clause 25 concerns risk of threats caused by improper protection against damage, fall or impurity during storage and transport to place of use

NOTE 2: Conformity assessment of product according to standard requirements refer to the scope of mechanical tests ordered by client

NOTE 3: During visual inspection before testing any visible defects that can have an effect on test results were not stated.

NOTE 4: Sample/object for testing was delivered to the Laboratory by the Orderer.

CONCLUSIONS:

Testing object **conforming** with requirements of PN-EN 12182:2012




TESTING

NORMATIVE REFERENCES

PN-EN 12182:2012

Technical aids for disabled persons – General requirements and test methods

PHOTO OF PRODUCT

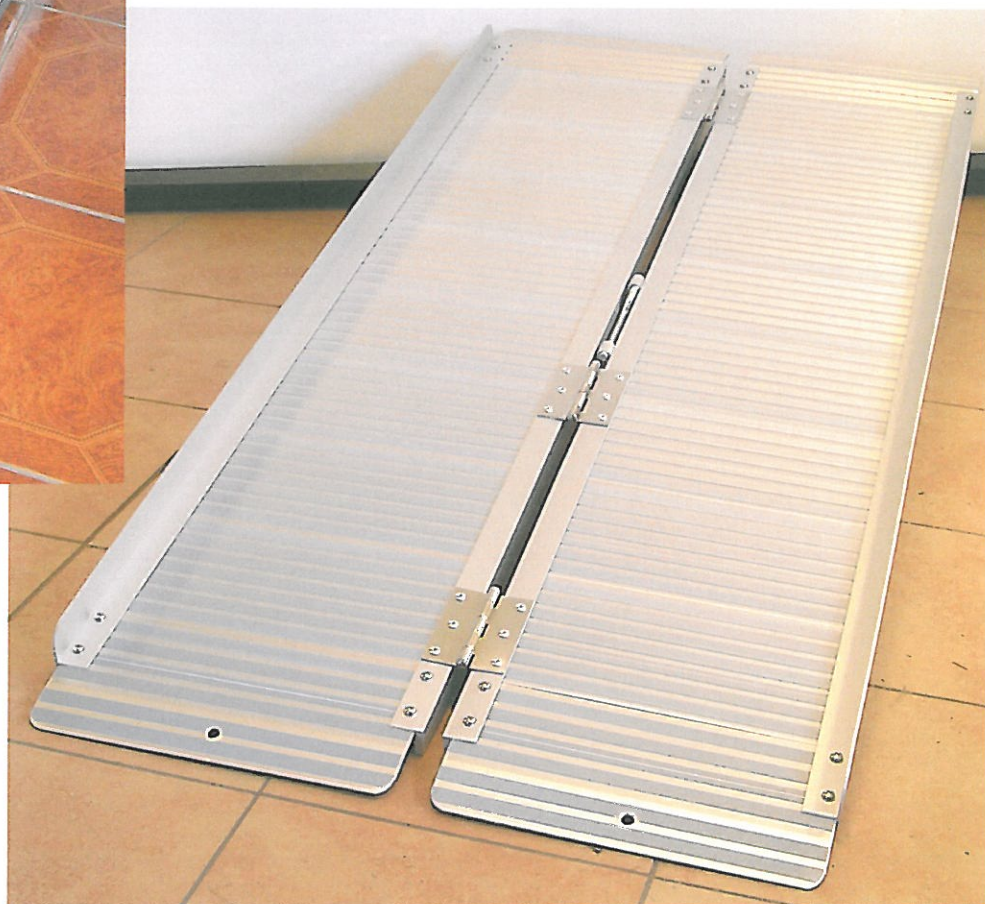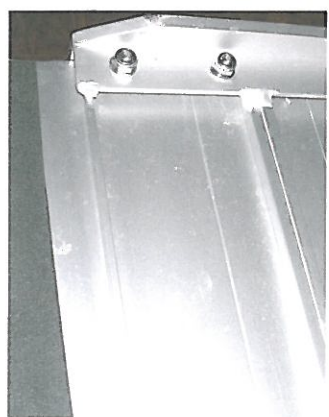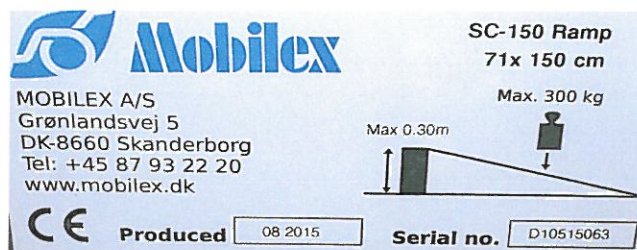

CHARAKTERISTICS OF PRODUCT

Name of product: SC – 150 Ramp	SN: D10515063	Max. loading: 300 kg	Mass of product: 14,06 kg
-----------------------------------	------------------	-------------------------	------------------------------

Dimensions:

Composite :	1531 mm x 352/366 mm x 85 mm
Spread out:	1531 mm x 707 mm x 55 mm

Material:

aluminum, steel, plastic

TEST RESULTS according to PN-EN 12182 : 2012

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Test result	Opinion	Comments
4.1	4.8, 5.2, 5.4.2, 5.5, 6, 8.2.1, 9.4, 10, 22, 24 i EN 1441	Risk analysis		--	N/T	
4.2	V/I	Expected characteristics and technical documentation		Conf.	Pos.	
4.3	EN ISO 14155	Clinic assessment		--	N/T	
4.4	V/I	Technical support which can be dismantled		Conf.	Pos.	
4.5	V/I	Single use connections		Conf.	Pos.	
4.6	V/I	Boundary values of user weight		Conf.	Pos.	
4.7	V/I	Immobilising means		--	N/A	
4.8	V/I, C5	Suitability of the product for people with cognitive impairment		--	N/T	
		The presence of the description in the manufacturer's documentation		--	N/T	
		Materials				
5.1	EN 60601-1-9	Recycling		--	N/T	
5.2	V/I, B 5.2	Flammability		--	N/A	
5.2.2	V/I	Upholstered parts, mattresses, bed bases and bedding		--	N/A	
5.2.3	V/I, EN 1021	Upholstered parts		--	N/A	
5.2.4	V/I, EN 597	Mattresses and bed bases		--	N/A	
5.2.5	V/I, EN ISO 12952	Bedding		--	N/A	
5.2.6	V/I, EN 60695-11-10	Moulded parts		--	N/A	
5.3	EN ISO 10993-1 Annex. D	Biological conformity and toxicity		--	N/T	
5.4	V/I	Contaminants and residues		--	N/A	
5.5	V/I, B.5.5.1	Microbiological infections and contamination	Cleaning	Conf.	Pos.	
	V/I, B.5.5.1		Disinfection	--	N/A	
	V/I, EN ISO 22442-1 B.5.5.2		Animal tissue	--	N/A	
5.6	EN ISO 9227	Resistance to corrosion		--	N/T	
6		Emitted sound and vibration				
6.1	EN ISO 3746 B6	Noise and vibration		--	N/A	
6.2	EN ISO 3746	Sound levels and frequencies of audible warning devices		--	N/A	
Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Real value	Test result	Comments
6.3	EN ISO 3746	Feedback		--	N/A	
7	EN 60601-1-2 7.2, 7.3, 7.4	Electromagnetic compatibility		--	N/A	
8		Electrical safety		--	N/A	
9	V/I	Overflow, spillage, leakage, and ingress of liquids		--	N/A	
10	V/I. Measur.	Surface temperature		--	N/A	$t^{\circ} \leq 41^{\circ}\text{C}$ ■ requirement does not concern heat of direct solar radiation - PN-EN 12182, clause 10a ■ requirement concerns only persons with insensitiveness of skin (who do not feel heat) - PN-EN 12182, clause 10d
11	V/I	Sterility		--	N/A	

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters	Real value	Test result	Comments
12	V/I. Measur.	Safety of moving parts	Conf.	Pos.	Note in service manual
13	V/I. Measur.	Prevention of traps for parts of the human body	Conf.	Pos.	Note in service manual
14	V/I	Folding and adjusting mechanisms	Conf.	Pos.	Note in service manual
15	V/I. Measur.	Carrying handles	Conf.	Pos.	loading 280N
16	V/I. Measur.	Assistive products which support or suspend users	Conf. *)	Pos.	loading 1,5x300kg=450kg, 70sek. 1000 cycles, 300kg
17	V/I. Measur.	Portable and mobile assistive products	--	N/A	
18	V/I, B 18	Surfaces, corners, edges and protruding parts	Conf.	Pos.	
19	B 19	Hand held assistive products	--	N/A	
20	B 20	Small Parts	Conf.	Pos.	
21	V/I. Measur. EN 60601-1	Stability	--	N/A	
22	B 22, V/I	Forces in soft tissues of the human body	--	N/A	
23	V/I. EN 614-1	Ergonomic principles	--	N/T	The requirements relate to the design process

*) Deformation – 25 mm, elastic deformation – 25 mm, sustained deformation – 0 mm

Pos. – positive; Neg – negative; N/T – not tested; N/A – not applicable; N/R – not required, N/O – not occurred, V/I.- visual inspection, Conf.- conformed.

NOTE 1: Assessment of package, clause 25 concerns risk of threats caused by improper protection against damage, fall or impurity during storage and transport to place of use

NOTE 2: Conformity assessment of product according to standard requirements refer to the scope of mechanical tests ordered by client

NOTE 3: During visual inspection before testing any visible defects that can have an effect on test results were not stated.

NOTE 4: Sample/object for testing was delivered to the Laboratory by the Orderer.

CONCLUSIONS:

Testing object **conforming** with requirements of PN-EN 12182:2012

-- END --